


Supplementary Figure 1: HPTLC plate view and chromatograms of GGE at 540 nm. Panel (A) represents track of sample and standard and (B)-(C) show chromatograms of the sample and standard at 540 nm

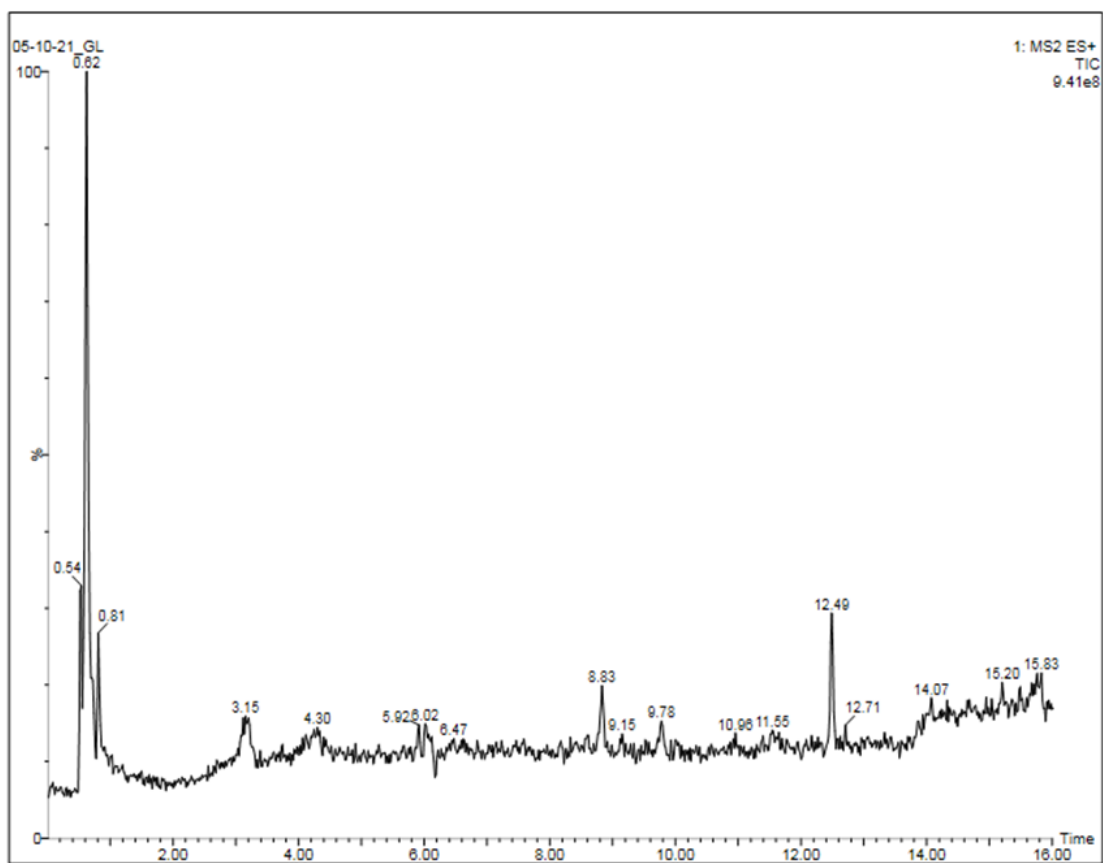

Supplementary Figure 2: UPLC-MS chromatogram of GGE